Print on Plain White Paper (Part No. 122919)

MIDMARK®

Installation/Operation Instructions

9A157001/002 SIDE RAIL ASSEMBLY (PAIR)

KIT COMPONENTS

Part Number	Description	Qty.
9A157001/002	Side Rail Assembly (Pearl Grey 001) or (Sand Grey 002)	1 pair
003-0579-00	Installation / Operation Instructions	1

REQUIRED TOOLS

None

INTRODUCTION

To provide patient security.

WARNING

Mount 9A157001/002 Side Rail on siderail bar of exam table. Maximum weight limitation on side rail panel is 20 lbs. (9.1 kgs.). Do not use with any other accessories on same side of table. Assure side rail is locked after positioning. Failure to comply may cause personal injury to patient.

INSTALLATION

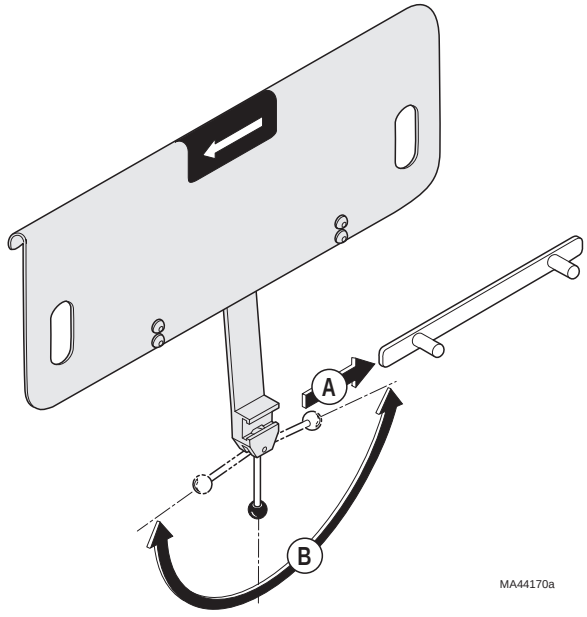

A. Slide clamp weldment onto side rail to desired position.

B. Rotate lock handle to one side to lock.

OPERATION

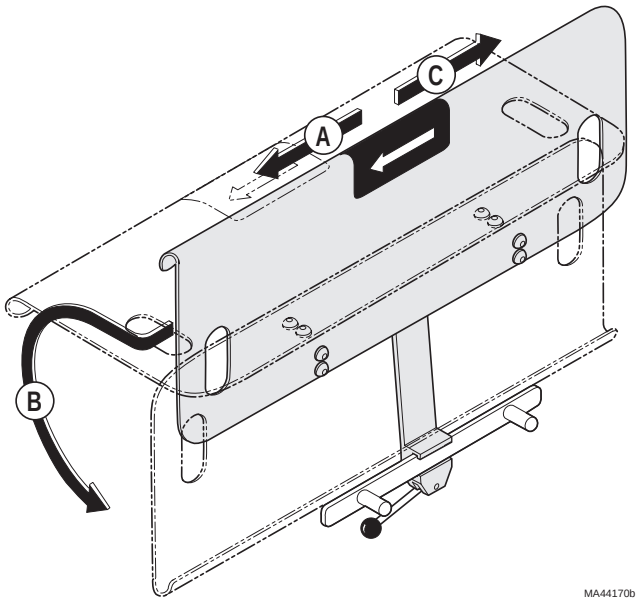

A. Pull side rail in direction of arrow, holding in that position.

B. Rotate side rail to desired position, straight out (90°) or down (180°).

C. Release side rail to lock.

WARNING

Assure side rail is locked in position.

MIDMARK®

Midmark Corporation, 60 Vista Drive, P.O. Box 286, Versailles, Ohio 45380-0286
Phone: 1-937-526-3662 Fax: 1-877-249-1793 midmark.com

003-0579-00 Rev. B (4/98)

© Midmark Corporation - 1998